



REPLACEMENT SHEET  
TITLE: "BLOOD SAMPLING DEVICE"  
SERIAL No.: 10/737,016  
ATTY: BRADLEY K. GROFF  
ATTY TEL: 770.984.2300  
ATTY DOCKET No.: 2G02.1-080

16/35

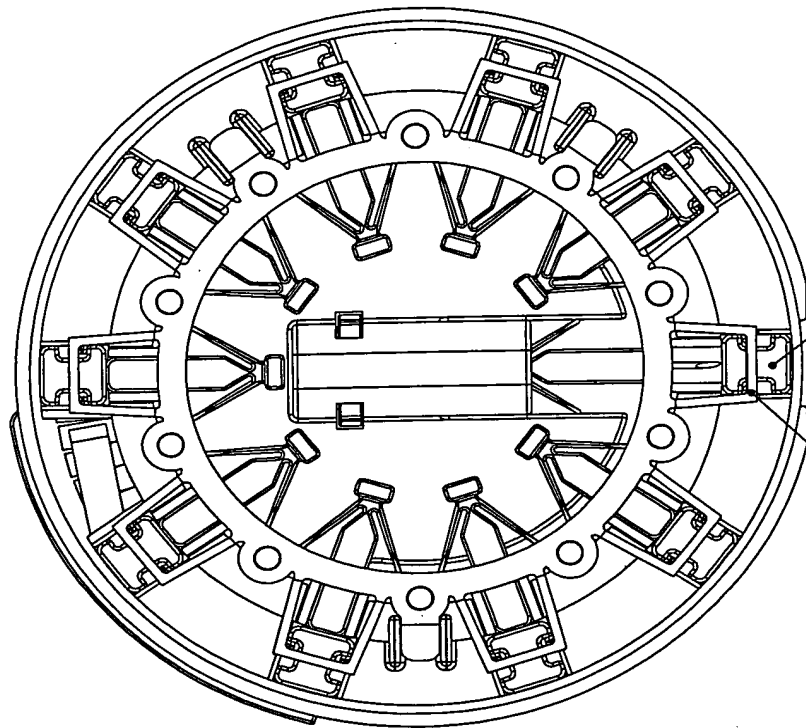


FIG. 26B

174  
176

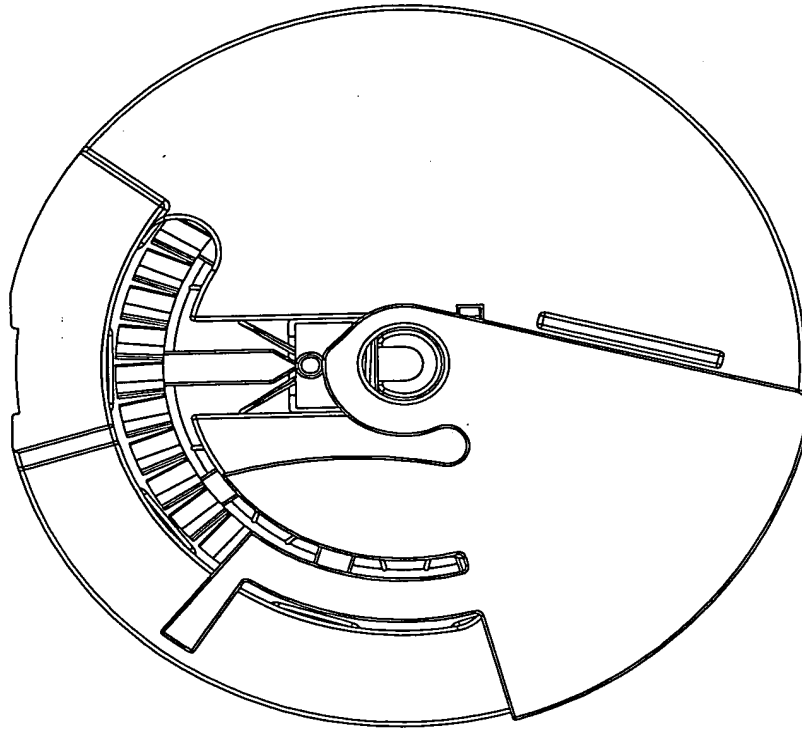


FIG. 26A

18/35

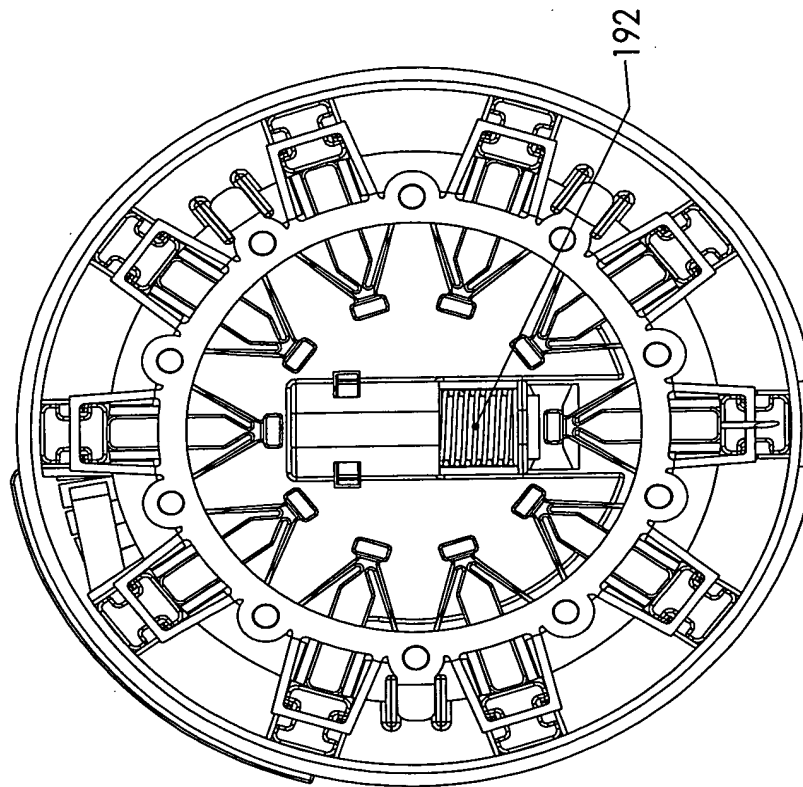


FIG. 28B

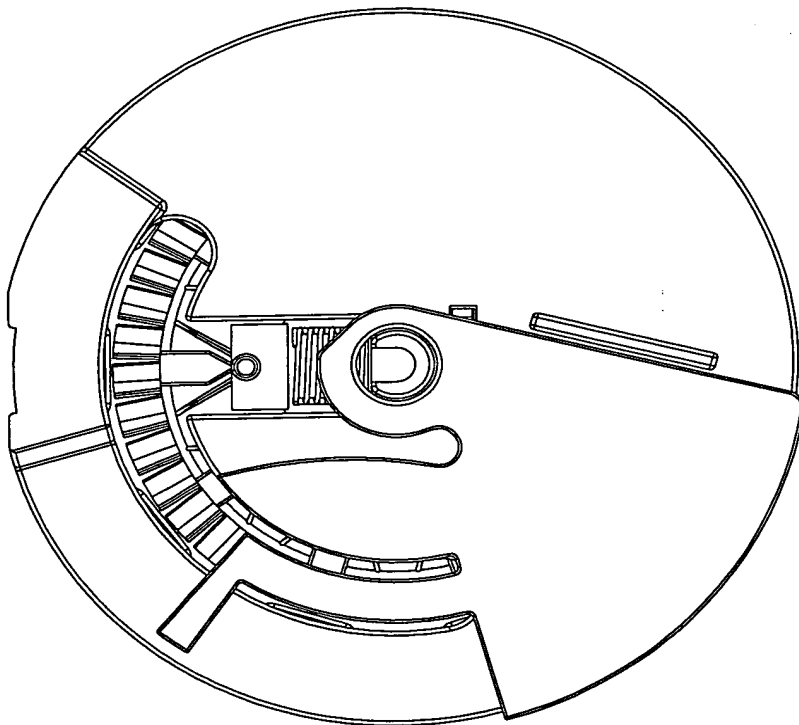


FIG. 28A

24/35

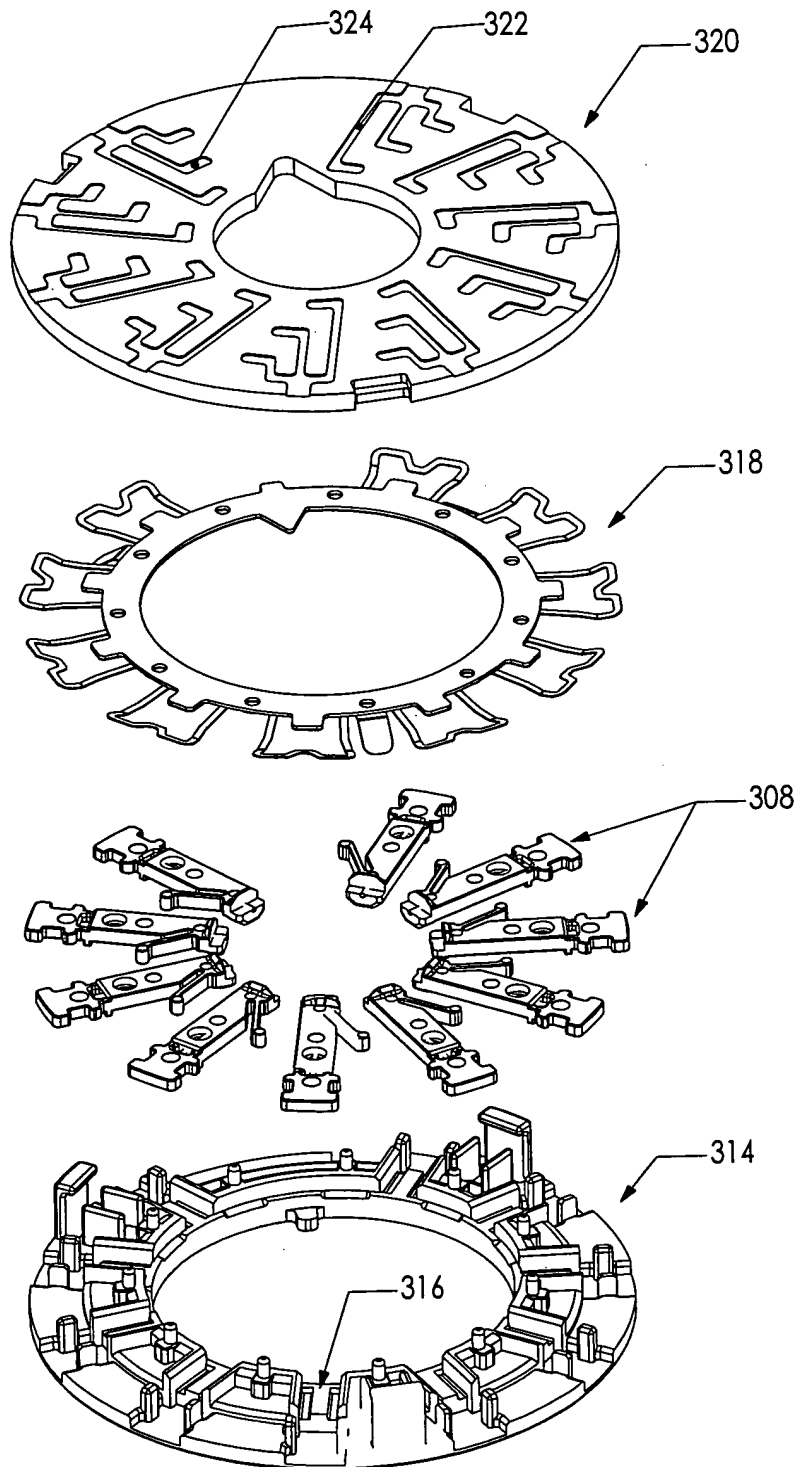


FIG. 35